


Jon Sterckx

Drumscapes

live percussion sampling

Technical Requirements

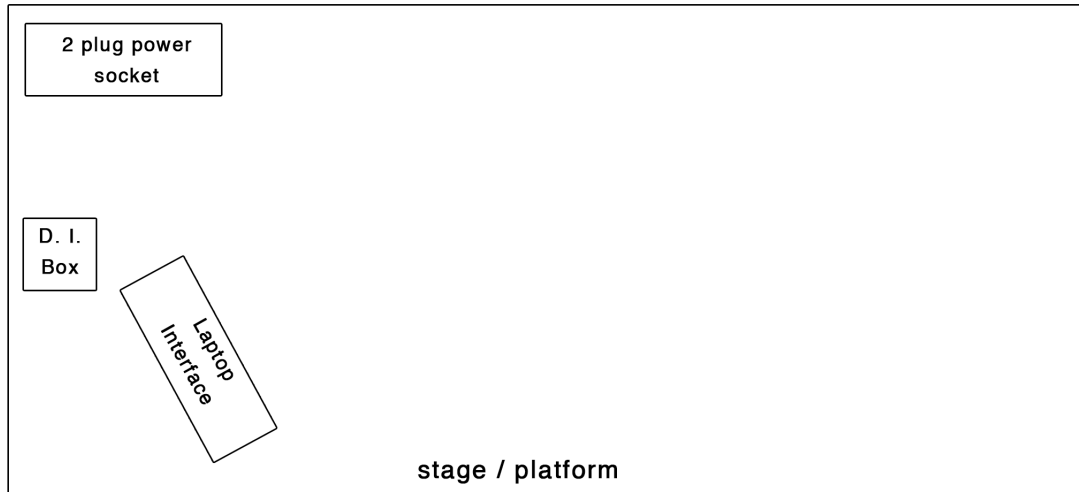

Audience

Stage minimum 7ft wide x 6 ft deep x 2 ft high / 2.15m x 1.85m x 60cm

PA for amplification with speakers forward of the stage. Mixer with multiband EQ.

4 socket power supply on stage & 2 x XLR output leads from my D.I box to your stagebox / mixer.

No monitors are required on stage. (monitoring with IEM)

I bring own mics, stands & their leads & D.I box.

Technician should be on desk throughout the performance.

Minimum 30 minutes required for set up & soundcheck.

Allow minimum 15 minutes to clear the stage after performance. Stage should be kept clear of other musicians / equipment etc until I have removed all equipment & instruments.

Parking for 1 vehicle.

Please contact with any queries:

Tel: 07913 665595
email: jon@drumscapes.net
web: www.drumscapes.net